

Moisture Probe Data Sheet

Customer Name:

Part Number: M2LRT

Serial Number: ??????-PR

Calibration Date: Dec.28, 2015


CALIBRATION

DUE DATE: Dec. 2017

NEW DATA

Calibration Date: Dec. 8, 2016

<u>ND #</u>	<u>MH</u>	<u>D.P. °C</u>	<u>MH</u>	<u>D.P. °C</u>	<u>D.P. °F</u>
0	0.2341	-110	0.2186	-110	-166
1	0.2399	-100	0.2271	-100	-148
2	0.2456	-90	0.2358	-90	-130
3	0.2515	-80	0.2449	-80	-112
4	0.2576	-70	0.2543	-70	-94
5	0.2724	-60	0.2701	-60	-76
6	0.2887	-50	0.2863	-50	-58
7	0.3138	-40	0.3100	-40	-40
8	0.3569	-30	0.3492	-30	-22
9	0.4281	-20	0.4189	-20	-4
10	0.5315	-10	0.5212	-10	14
11	0.6919	0	0.6879	0	32
12	0.9402	10	0.9505	10	50
13	1.2776	20	1.3133	20	68

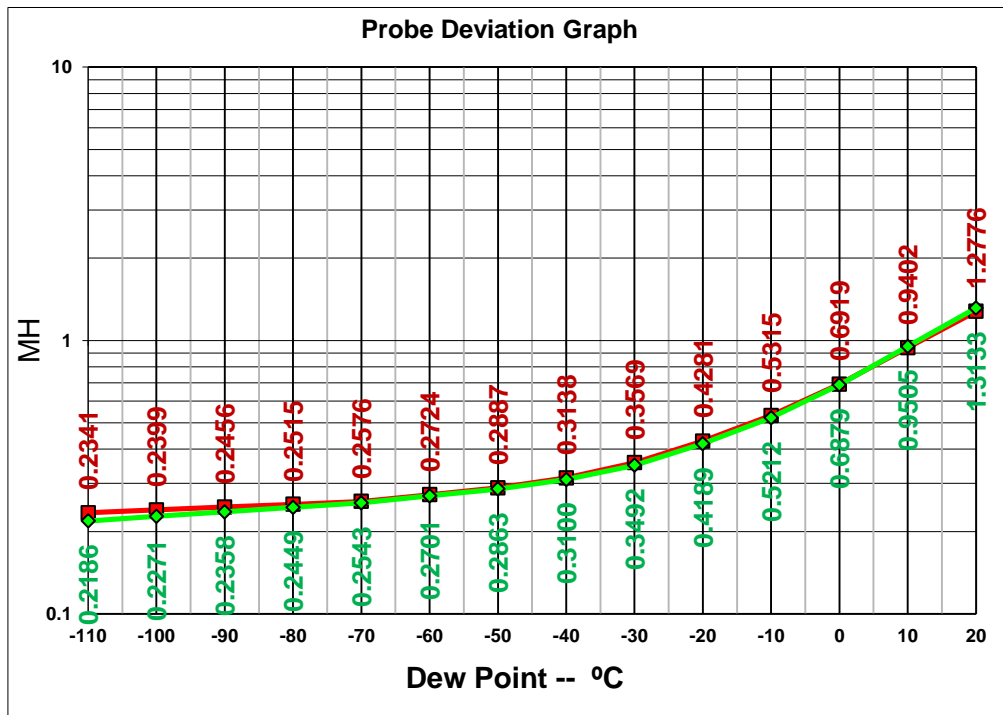

REV.:2 April 14, 2013